
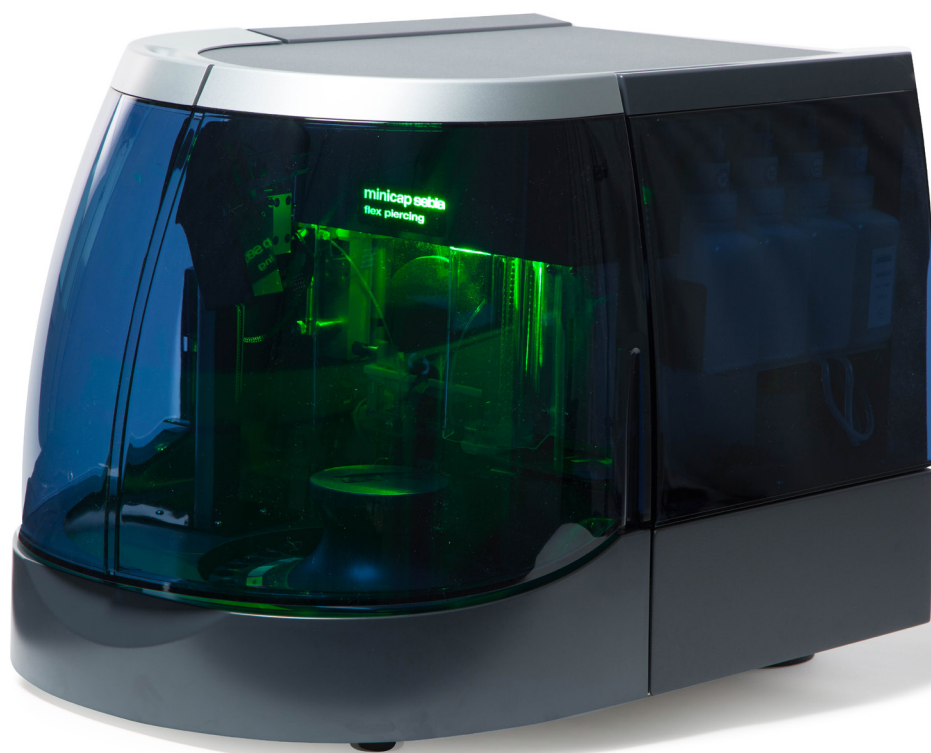


MINICAP *FLEX-PIERCING*

MULTI-ASSAY SOLUTION
FOR AUTOMATED
ELECTROPHORESIS



sebia 
The new language of life

Multi-assay instrument


Extended test menu

- Serum Protein Electrophoresis (SPE)
- Serum Immunotyping
- Hb A1c
- Hemoglobin Electrophoresis
- CDT/CDT_{IFCC}


Capillary Electrophoresis

Analytical performance


- Fast protein separation
- Excellent resolution and reproducibility

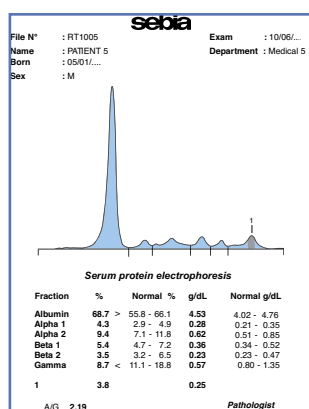


PROTEIN(E) 6

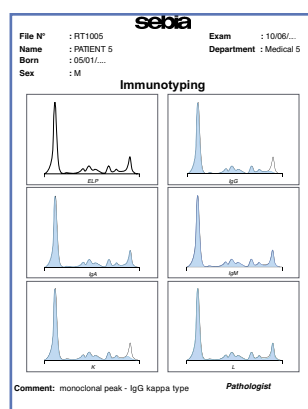


IMMUNOTYPING

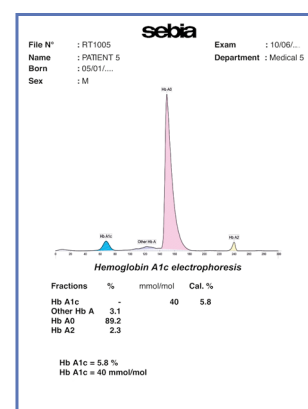


HbA1c

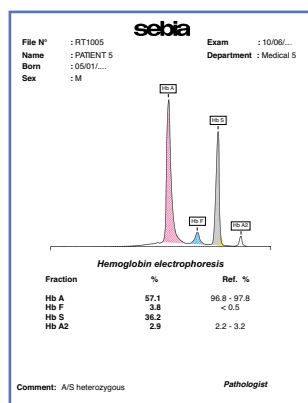

HEMOGLOBIN(E)

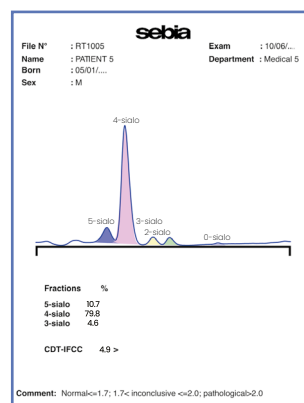

CDT, CDT_{IFCC}



Sample processing


Fully automated

- Sample mixing and cap piercing capabilities with whole blood techniques
- Full traceability from primary tube to final result

IT integration

Efficient information flow

- Networking of all Sebia instruments
- Remote validation of the results
- Off-site remote access
- Unlimited data storage



Interpretation software


and results validation

- Intuitive and user-friendly interface
- Multicriteria search function
- Automatic recall of patient's history
- Automatic triage of the results

Performance

High throughput

- SPE: 18 tests/h
- Hb A1c: 8 tests/h
- Hemoglobin: 7 tests/h
- CDT & CDT_{IFCC}: 10 tests/h

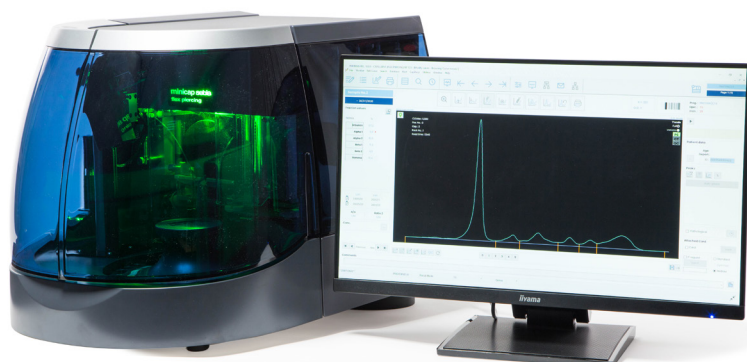

Specifications

- Reduced footprint
- Maximum sample loading capacity of 28 samples

Ordering information

Instruments

- MINICAP FLEX-PIERCING1232

Reagents

- MINICAP PROTEIN(E) 62203
- MINICAP HEMOGLOBIN(E)2207
- MINICAP CDT2208
- MINICAP Hb A1c2215
- MINICAP IMMUNOTYPING2300

Accessories

- BARCODES READER
CAPILLARYS / MINICAP1079

Consumables

- MINICAP FLEX-PIERCING
CAPICLEAN2251
- MINICAP
REAGENT CUPS / 125 (3)2281
- MINICAP
LIDS FOR USED CUPS BINS (12)2286
- CLEAN PROTECT2059



Scan here
for more
information on
MINICAP FLEX-PIERCING

For further information, please find your Sebia local representative to
contact on our Website www.sebia.com/sebia/worldwide-presence/.



Sebia | RCS Evry 672 041 902 | Parc technologique Léonard de Vinci | 27, rue Léonard de Vinci | CP 8010 Lisses | 91008
Evry cedex | France | Tel.: +33 1 69 89 80 80 | E-mail: sebia@sebia.com | www.sebia.com

©2026 **Sebia** - RCS Evry 672 041 902 | Parc technologique Léonard de Vinci | 27, rue Léonard de Vinci | CP 8010 Lisses | 91008 Evry cedex | France - Ref: MFPBIEN - 03/2023
Non-contractual illustration - Sebia reserves the right to modify at any time and without notice the information contained in this document intended for healthcare
professionals. This document contains information intended for wide distribution and may therefore contain product details or information that is not available or valid in your
country. Carefully read the instructions in the reagent package inserts and instrument manuals.